CONFYCARE®



# FIX-MT2 SERIES

## FIX-MT2 / FIX-MT2D3 with Drawer

# INSTALLATION MANUAL

Assembly of your new free standing table is very simple and tool free. Please see the following steps.

- Remove all bubble wrap and ties from from the table to leave the legs and the table exposed.
- Stand over the table. Hold one side of the table legs and pull them slowly upward until they are vertical.
- Slowly lower the table legs into the brackets on each corner of the table.
- Line up the pin and the groove then push the table into place. Put extra force once onto the leg bars once in position so it slots tightly and deep into the groove.
- Repeat on the other end of the table.
- Turn the table over onto its legs and give an extra push on each end of the table once free standing to make sure it's locked in the right place.
- For the head section insert the metal U shaped bar into the grooves on the back of the head section to the desired angle. Remove the U shaped bar from the grooves completely to lower it to a flat position.

## 1. Table leg installation



The table is shipped completely assembled. (Figure 1)

Figure 1



Figure 2


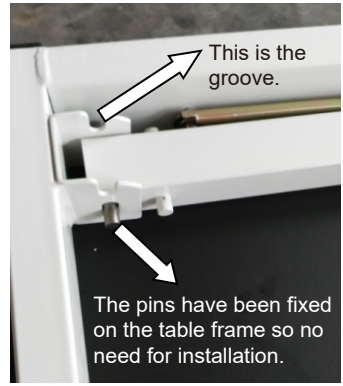



Figure 3

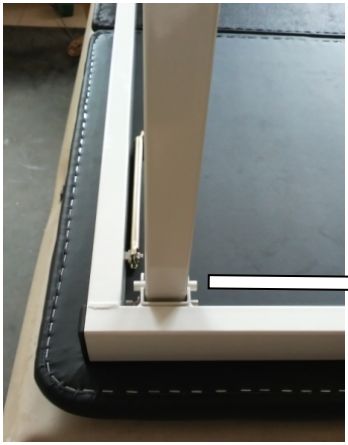

Lift the table leg and line up the pin into the groove then put extra force onto the leg bars once in position so it slots in tightly and deep into the groove.(Figure 4)

Figure 4

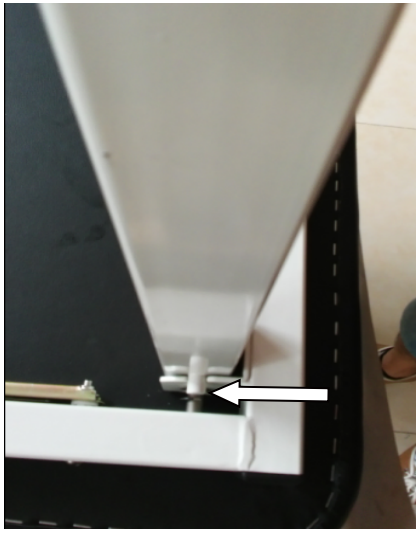


Figure 5



Figure 6

Turn the table over on it's legs and give an extra push on each end of the table once free standing to make sure it is locked in the right place. (Figure 5 & 6)

## 2. Table drawer installation



Figure 7

This is a table that has been installed. Please put the table on it's legs. The drawer track has been fixed on the table frame so just need to insert the drawers into the table. (Figure 7)



Figure 8

The table frame and drawer are separate packages.There are total 3 drawers. Please remove the drawers from their boxes. (Figure 8)



Figure 9

Please insert the drawers into the track by hand. It is very easy to locate the correct place. Please check the drawer function after installation. (Figure 9)



Figure 10

Here is the drawer installation completed. Please check the table image for your reference of correct installation. (Figure 10)

**Legend to symbols and information on the product label.**

- **Model**: Product identification.
- **Model Num**.: Product version.
- CE : CE conformity marking.
- MD : Medical Device
- SN : Unique serial number identifying the product.
-  : Date of manufacture.
- **Product Net Weight** : Table weight in kg.
-  : Consult the instructions for use or the user guide.
- **Max. Load** : Maximal load capacity that the table can support.
-  : Manufacturer identification.
- EC REP : Authorized representative in the EU.
-  : Importer.

## TROUBLESHOOTING

If, during the life of the table you detect any malfunction or need a repair, contact your dealer and do not use the table until you have received a diagnosis or the table has been professionally repaired.

## MAINTENANCE

Carry out a visual inspection at least once a month to check the general conditions of the table. Moreover, you must do the following:

- Check the correct adjustment of the different sections.
- Check and clean the table frame.
- Check and tighten screws (if necessary).
- Grease the parts with friction.

## RECYCLING

If you need to dispose of the table or any of its parts or accessories, consult and respect the laws and regulations applicable to waste management and protection of the environment.

## Contraindication

Please note that our beds are not sterilized. Please do not use them according to aseptic standards.

## WARRANTY

This warranty shall remain in effect for 3 years for the structure and 1 year for accessories from the date of original consumer purchase. An original sales receipt or proof of purchase may be required in order to redeem the warranty.
All repairs to the Product must be performed by a service center certified by Coinfycare. Any modifications or repairs performed by unauthorized centers or groups will void this warranty. This statement of guarantee prevails over any other statement specified or implied by the seller.

## CLEANING AND DISINFECTION

Dust the table with a soft, dry cloth.

To clean the upholstery, apply a solution of warm water and a mild detergent (for example, neutral soap) with a well wrung soft cloth. Wipe the table over once cleaned.

Disinfect upholstery and other surfaces with a suitable bactericide for this purpose.

Apply the disinfectant on a soft cloth, never directly on the table.

Never use a mixture of disinfectants or a mixture of disinfectant and soap.

Wipe the table upholstery over once cleaned & disinfected with a cloth and water only. This will remove any residue from the upholstery.

Avoid the accumulation of moisture on the moving parts of the metal structure, as they could rust.

Since we do not know which disinfectant will be used, we cannot guarantee that it will not cause damage to the upholstery. Read the instructions and warnings for use of the disinfectant product carefully before its purchase or use.

## TRANSPORTATION AND STORAGE CONDITION

**Transport condition**

The products can be transported by general means of transportation. They should be protected from the sun and rain, and should not be mixed with toxic, harmful and corrosive materials.

**Storage**

The packed table should be stored in a dry and well ventilated environment without corrosive gas.

## CONTACT

Applicant / company name / after sales service unit:

Huangshan Jinfu Medical Equipment Co., Ltd
Domicile / production address: No. 17,
Qiliting, Qimen County, Huangshan City,
Anhui Province China
Tel: 0086 571 87006218
www.coinfycare.com

European legal representative:
LOTUS NL B.V.
Koningin Julianaplein 10, 1e Verd 2595AA,
The Hague, Netherlands

CONFYCARE®